



Copy of 5 Laser B3 V2 UV2 R3 YG5

Cytometer:	FACSAriaII	User:	Christiane
Cytometer Name:	FACSAriaII	Institution:	IU-Bloomington
Serial Number:	1	Software:	BD FACSDiva 9.0.1
Input Device:	Manual	Date:	5/20/2022 2:03:44 PM
Sheath Pressure:	20.00		
Nozzle Size:	100		
Window Extension:	4.00		


BLUE Laser
(488nm)
FSC

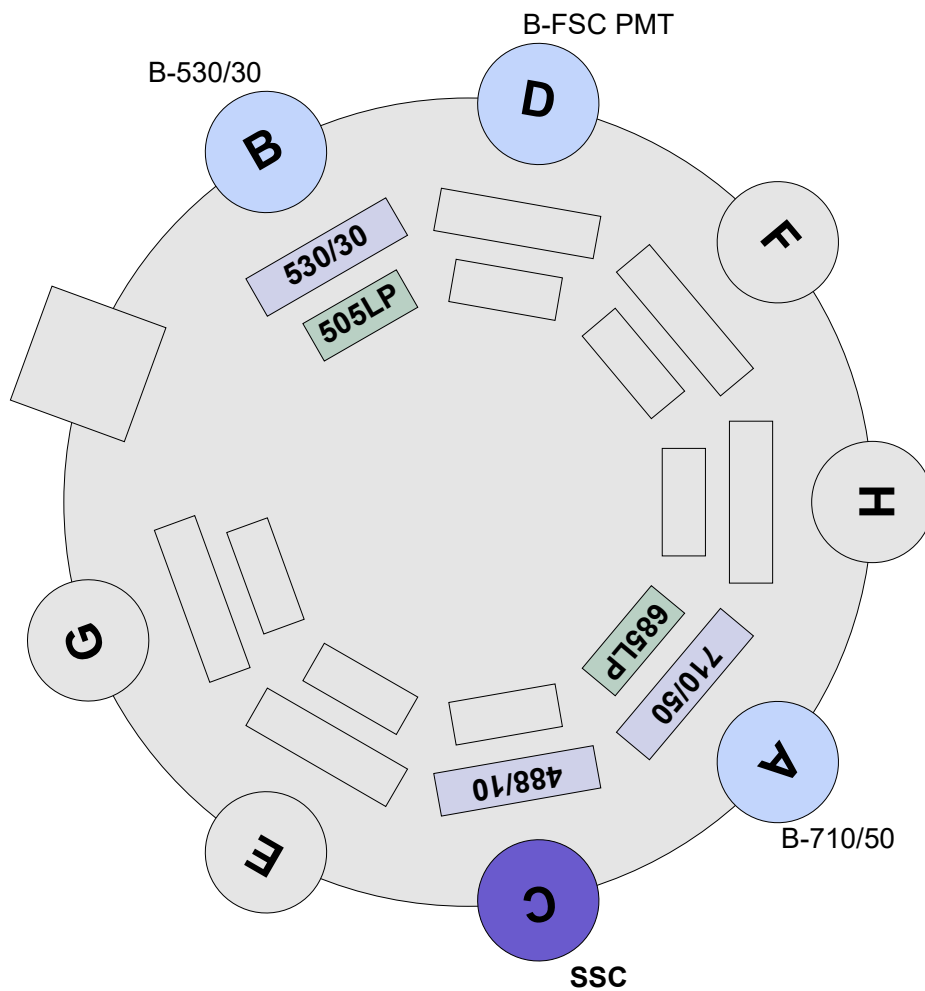


VIOLET Laser
(405nm)

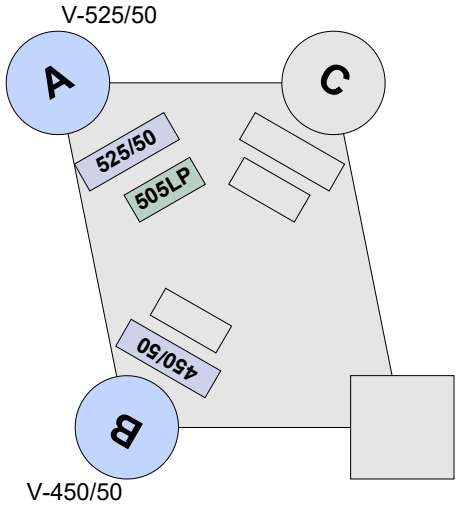


UV Laser
(355nm)

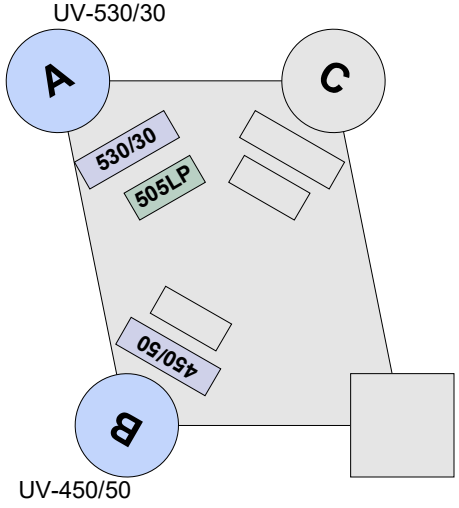

RED Laser
(640nm)

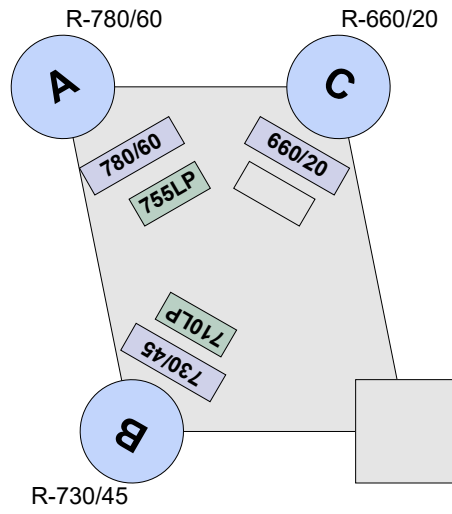

YG Laser
(561nm)

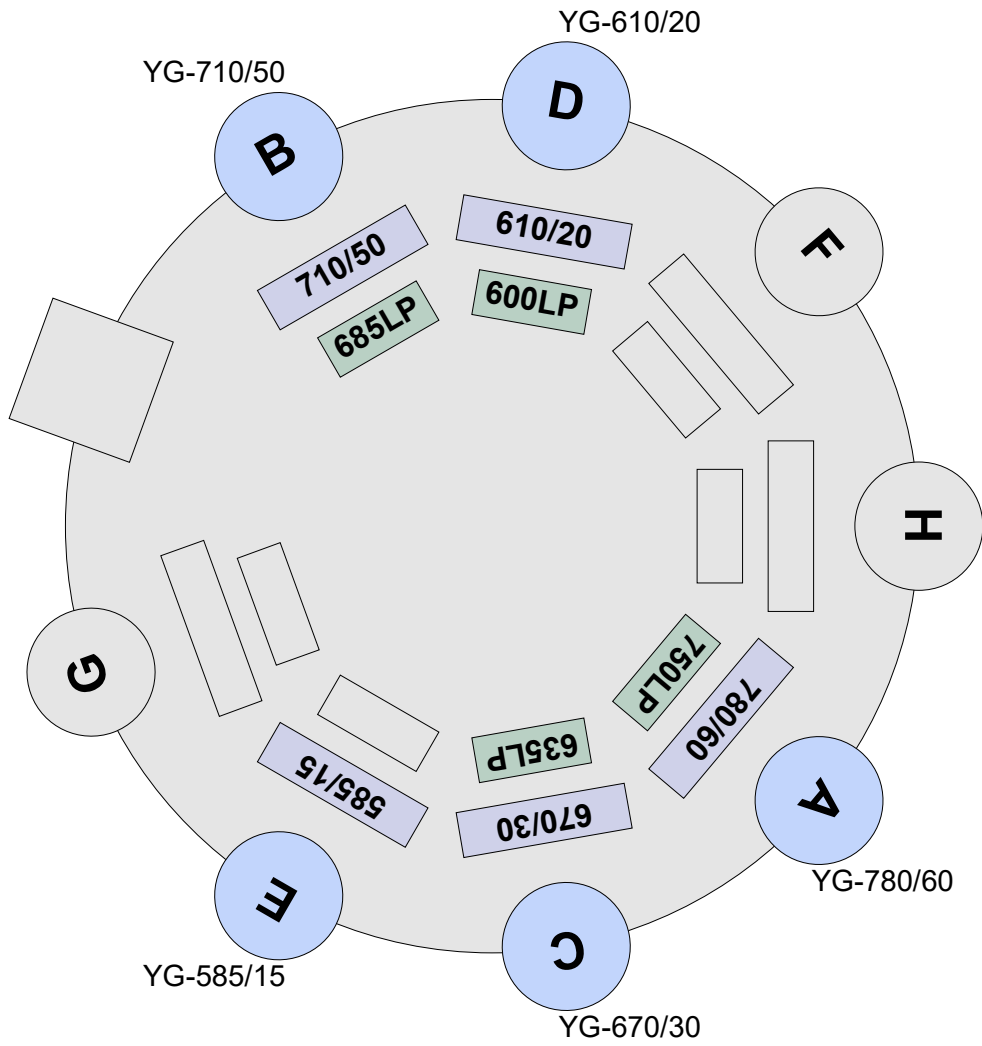

Comments: